


LEVEL
18.10.2009
20:59:31

Output: Analog
Imp: 600Ohm
Sine
0.00dBV 250.0 Hz

Input: Analog
Imp: 100kOhm
A: -5.92dBV 249.9 Hz

Filter:
Off

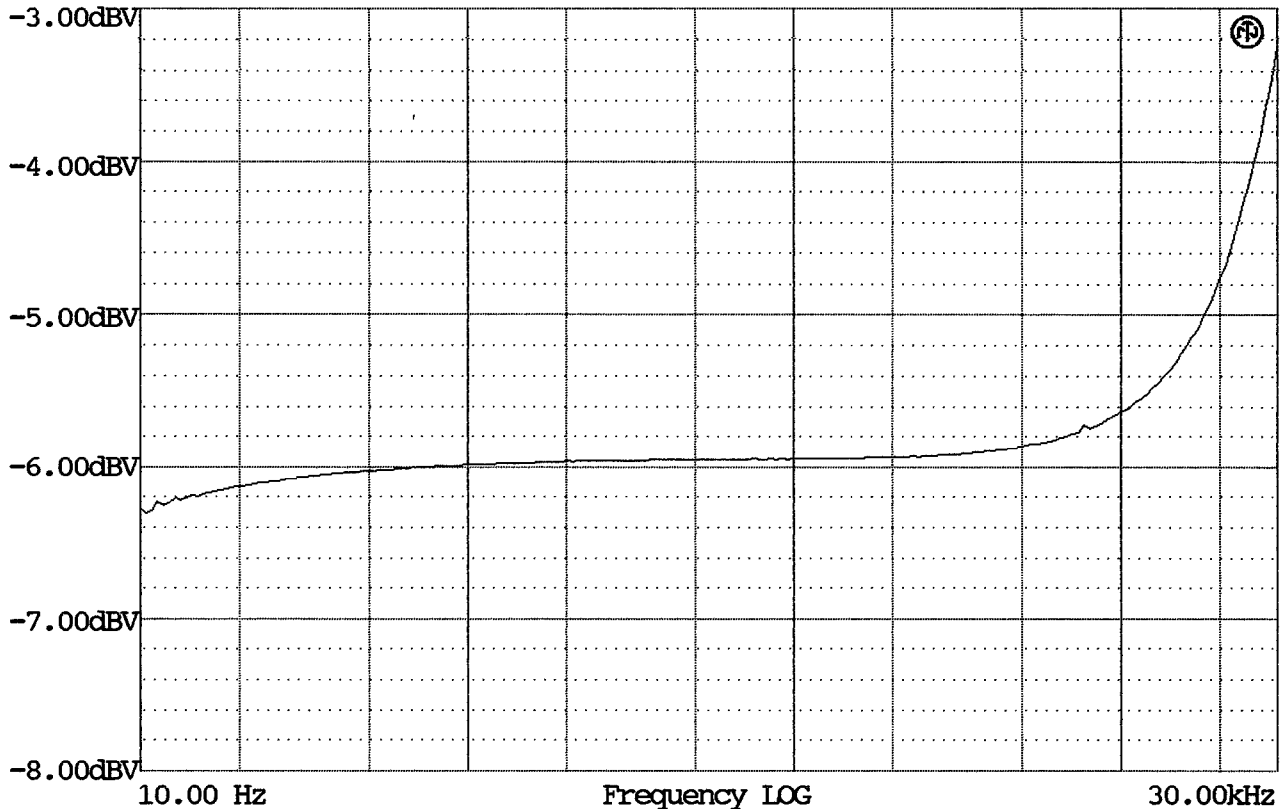


THD+N
18.10.2009
22:42:46

Output: Analog
Imp: 600Ohm
Sine
0.00dBV 250.0 Hz

Input: Analog
Imp: 100kOhm
A: -5.95dBV 249.9 Hz

Filter:
AUDIOBP

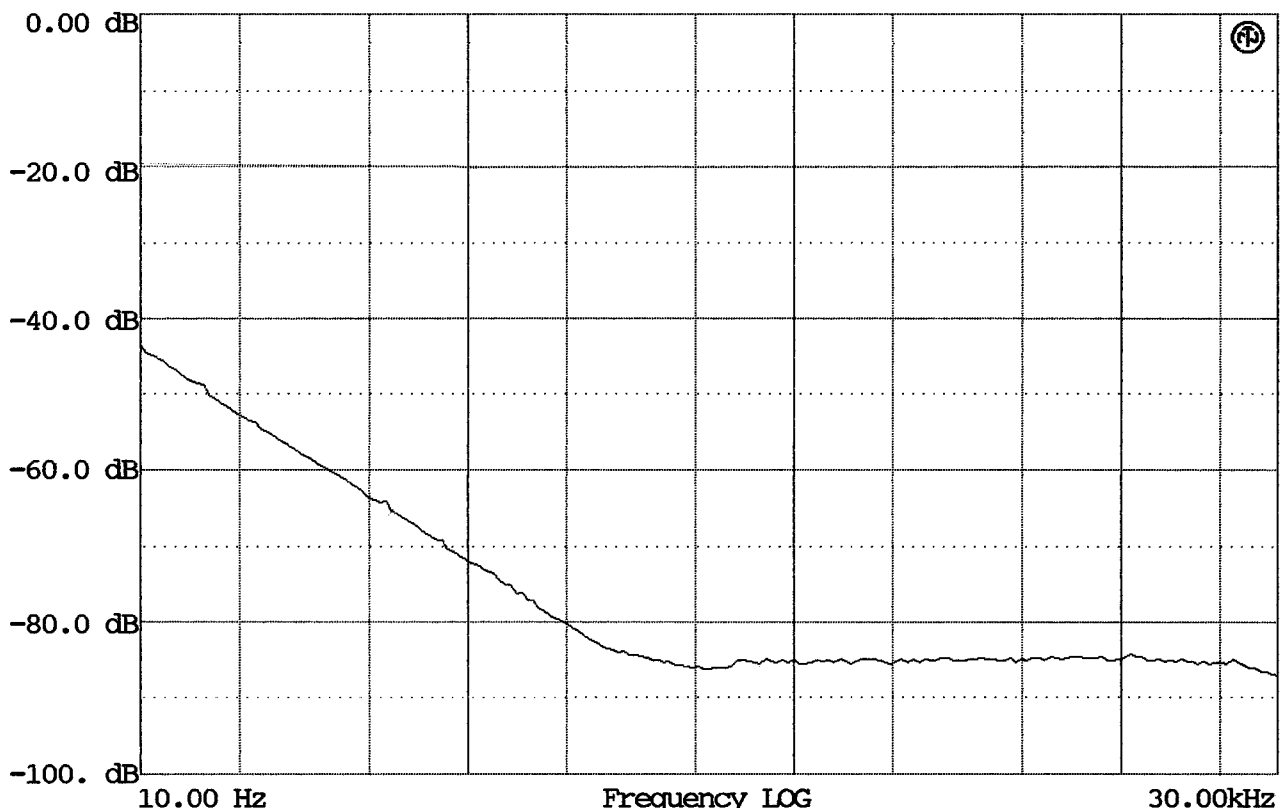

NEUTRIK NIM 4


THD+N
18.10.2009
22:49:02

Output: Analog
Imp: 600Ohm
Sine
10.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: 4.03dBV 249.9 Hz

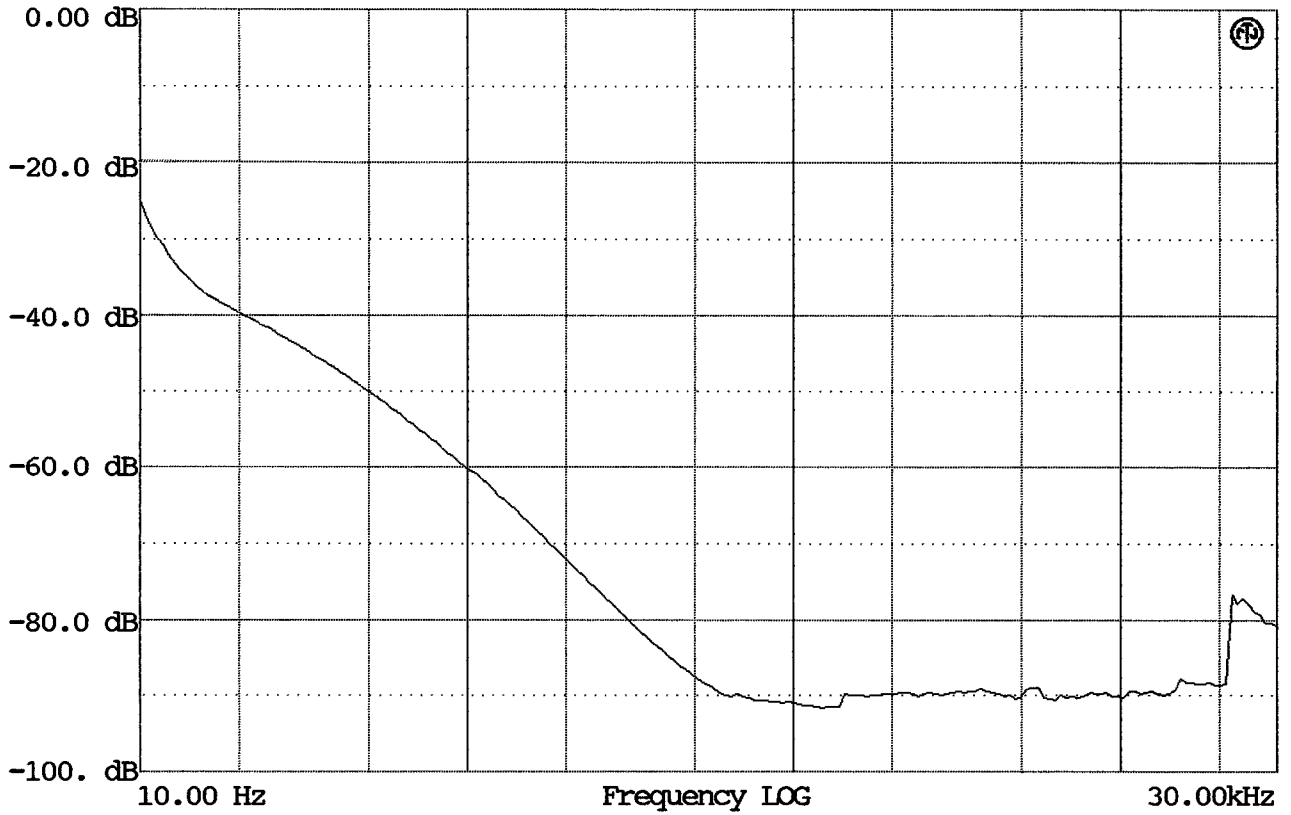


THD+N
18.10.2009
23:20:58

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: 14.0dBV 249.9 Hz

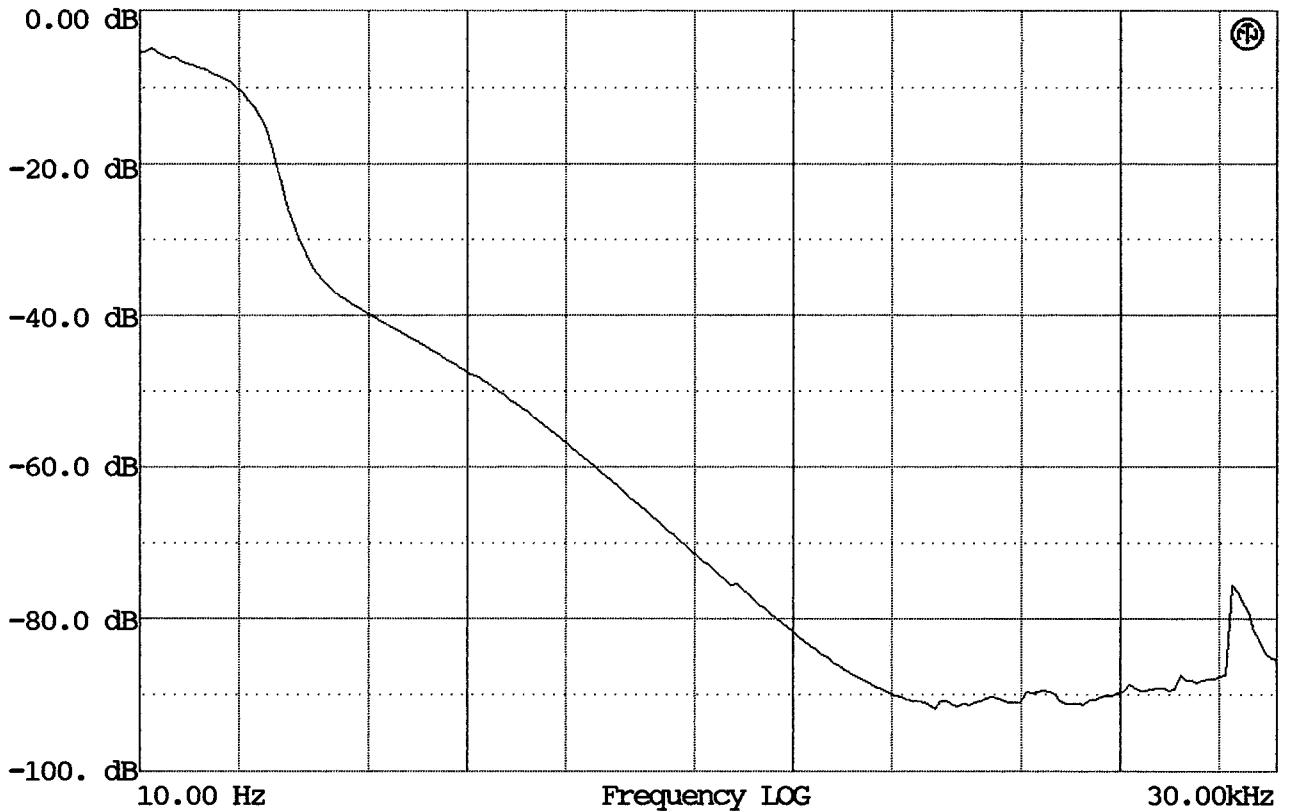

NEUTRIK NTM 4